


<b>Title:</b>	<b>UCI BL600 BCR Set-Up</b>	<b>ID:</b>	
		0058	
<b>Date in:</b>	<b>Response:</b>	<b>Model:</b>	<b>Author:</b>
2008-02-19	2008-02-19	LPX	CMa


## UCI BL600 BCR Set-Up

On LPX, LPR units with UCI feature installed remove Back Panel prior pulling Controller Module from side of the instrument.

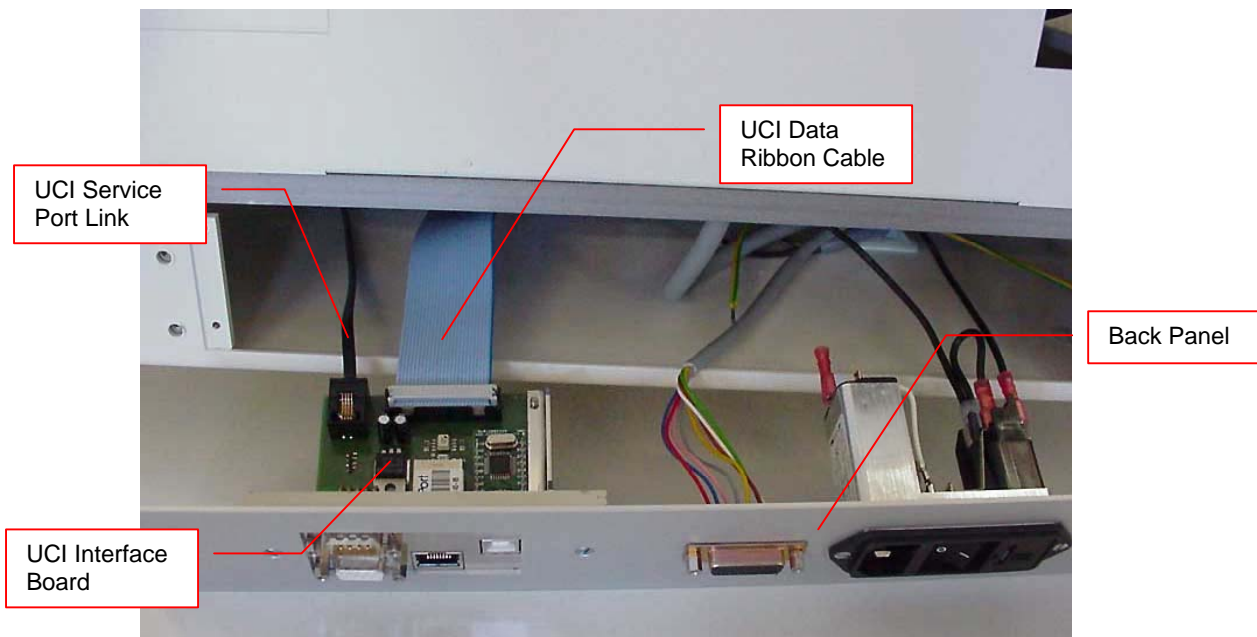

Remove UCI Data Ribbon cable and pull out Controller Module plate from front side

RJ45 BCR connector

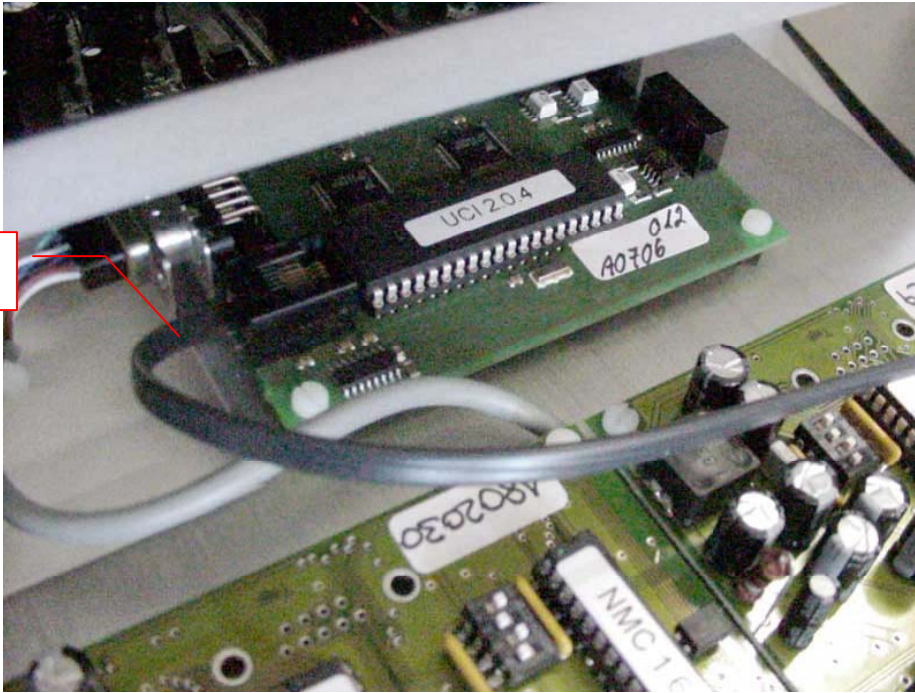

BCR to PC Service Cable

RJ12 BCR connector

